
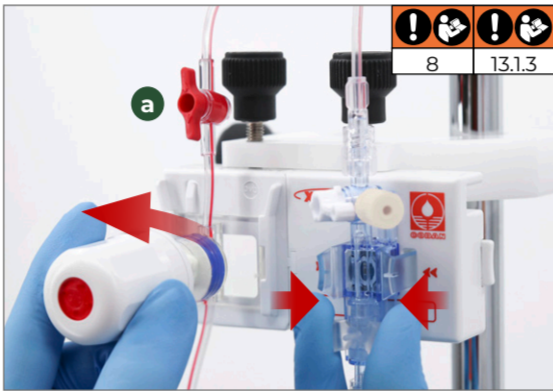
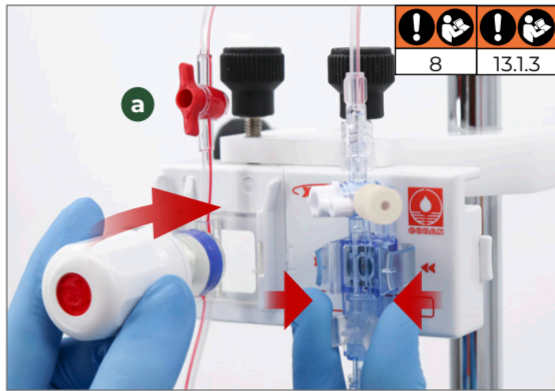









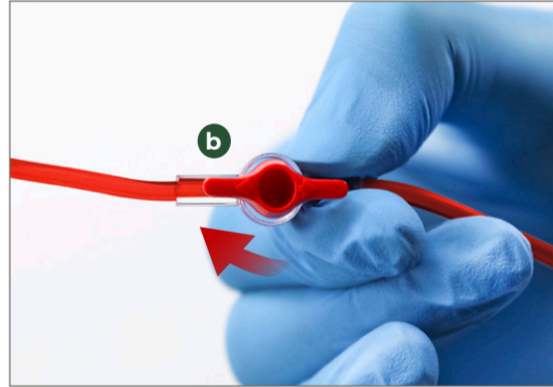




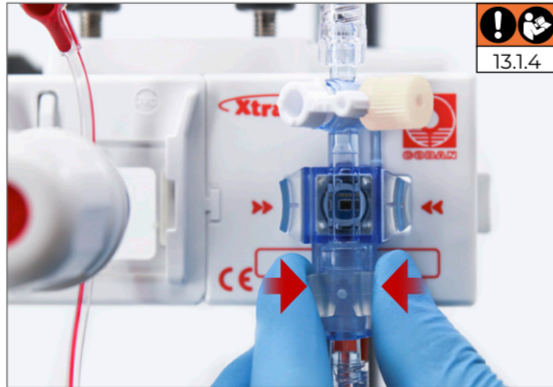
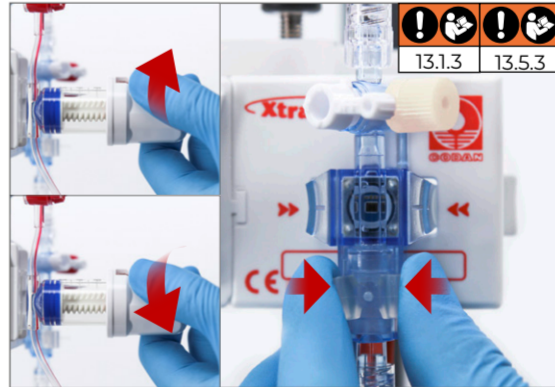
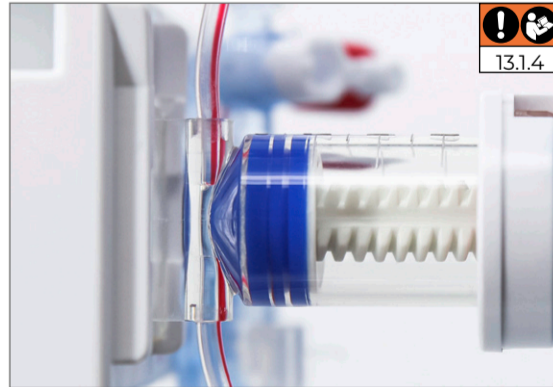


I. Preparation / priming ABSS^{XL}

Set	Reservoir	Sampling port
 <p>1 Prime pressure monitoring set.</p>	 <p>2 When filling the reservoir, open it slowly 3/4 of a turn (270°) anticlockwise and then close again.</p>	 <p>3 Prime sampling port completely and free of air bubbles.</p>

II. Blood sampling with the ABSS^{XL}

 <p>1 Disinfect sampling port. Pay attention to flash-off time!</p>	 <p>2 Close 1-way stopcock.</p>	 <p>3 Completely open reservoir slowly by turning anticlockwise.</p>	 <p>4 Connect the withdrawal container and the withdrawal adapter.</p>	 <p>5 Puncture the withdrawal adapter incl. the withdrawal container.</p>
 <p>6 Draw blood sample.</p>	 <p>7 Close 1-way stopcock.</p>	 <p>8 Remove the withdrawal adapter with the withdrawal container.</p>	 <p>9 Disinfect sampling port.</p>	 <p>10 Open 1-way stopcock.</p>

III. Reinfusion & flushing

 <p>1 Completely close reservoir slowly by turning clockwise.</p>	 <p>2 Open 1-way stopcock.</p>	 <p>3 Flush the ABSS^{XL}.</p>	 <p>4 Open reservoir slowly 3/4 of a turn (270°) anticlockwise and then close again.</p>	 <p>5 Visual inspection: Flush until all blood residue is removed.</p>
 <p>6 Flush the ABSS^{XL}.</p>	 <p>7 Control: Check pressure monitoring & display on monitor.</p>			



This Quick Guide illustrates the most important steps and is no substitute for following the instructions for use. Always read and follow the information regarding the intended use as well as the warnings and safety instructions given in the instructions for use. The references in the individual steps indicate the corresponding section and respective warnings in the instructions for use. If these instructions are not observed/complied with, there are significant safety risks for patients, users and third parties. Observe the hygiene regulations in your facility.

